

Fig. 1

STORAGE AREA FOR:  
AED SHOCK PADDLE ELECTRODES  
AND OXIMETER ELECTRODE  
(NONE SHOWN FOR CLARITY)

STORAGE AREA FOR:  
AED SHOCK PADDLE ELECTRODES  
AND OXIMETER ELECTRODE  
(NONE SHOWN FOR CLARITY)

OXYGEN CYLINDER,  
REGULATOR, GAUGE,  
MASK AND HOSE  
(MASK AND HOSE  
NOT SHOWN  
FOR CLARITY)

SPEAKER

REAR STORAGE AREA  
FOR DC BATTERY,  
(TERMINAL WIRES IN  
BACK COMPARTMENT)

OXYGEN AND  
PULSE DISPLAY  
FOR OXIMETER


VOICE PROMPT  
SELECTION/CONTROLS

OXIMETER CONTROLS

AED CONTROLS

LCD SCREEN

Fig. 2

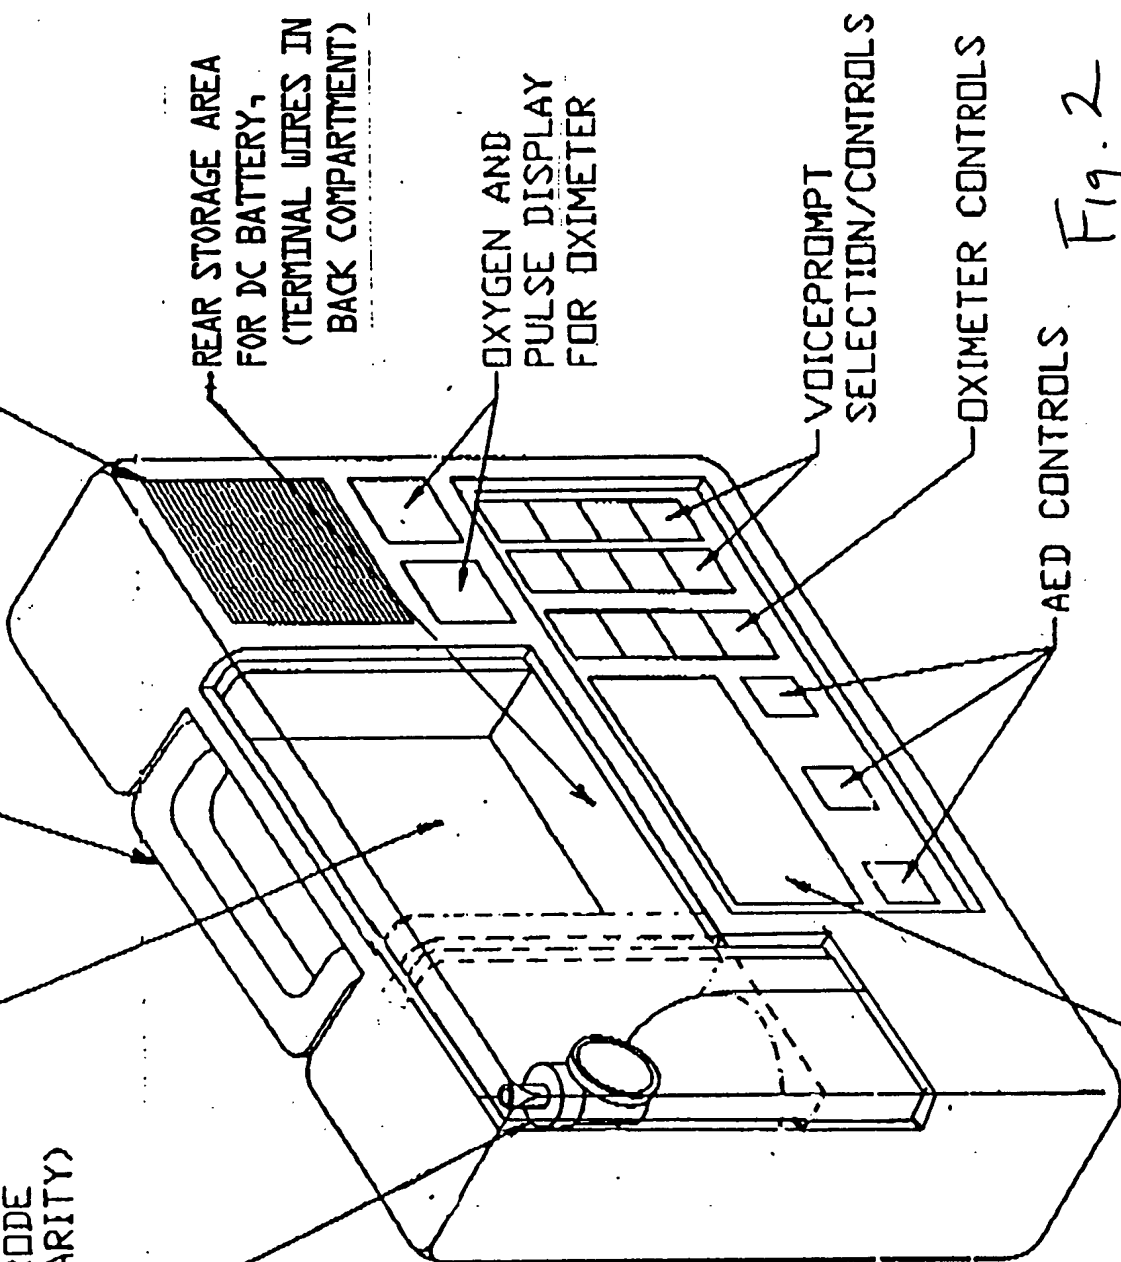

STORAGE AREA FOR:  
AED SHOCK PADDELE ELECTRODES  
AND OXIMETER ELECTRODE  
(NONE SHOWN FOR CLARITY)

OXYGEN CYLINDER,  
REGULATOR, GAUGE,  
MASK AND HOSE  
MASK AND HOSE  
NOT SHOWN  
FOR CLARITY)

ALSO NOT SHOWN:  
ELECTRO-MECHANICAL ON/OFF,  
LITER FLOW-CONTROL,  
PRESSURE CONTROL, AND  
LITER FLOW/PRESSURE/TIME  
SEQUENCING (VENTILATOR)

HANDLE

SPEAKER

REAR STORAGE AREA  
FOR DC BATTERY,  
(TERMINAL WIRES IN  
BACK COMPARTMENT)

OXYGEN AND  
PULSE DISPLAY  
FOR OXIMETER

VOICEPROMPT  
SELECTION/CONTROLS

OXIMETER CONTROLS

AED CONTROLS

LCD SCREEN

--- CARDIO-DIAGNOSIS & MONITORING  
--- RESPIRATORY DIAGNOSIS & MONITORING  
--- USER INSTRUCTIONS & PROMPTS

Fig. 3

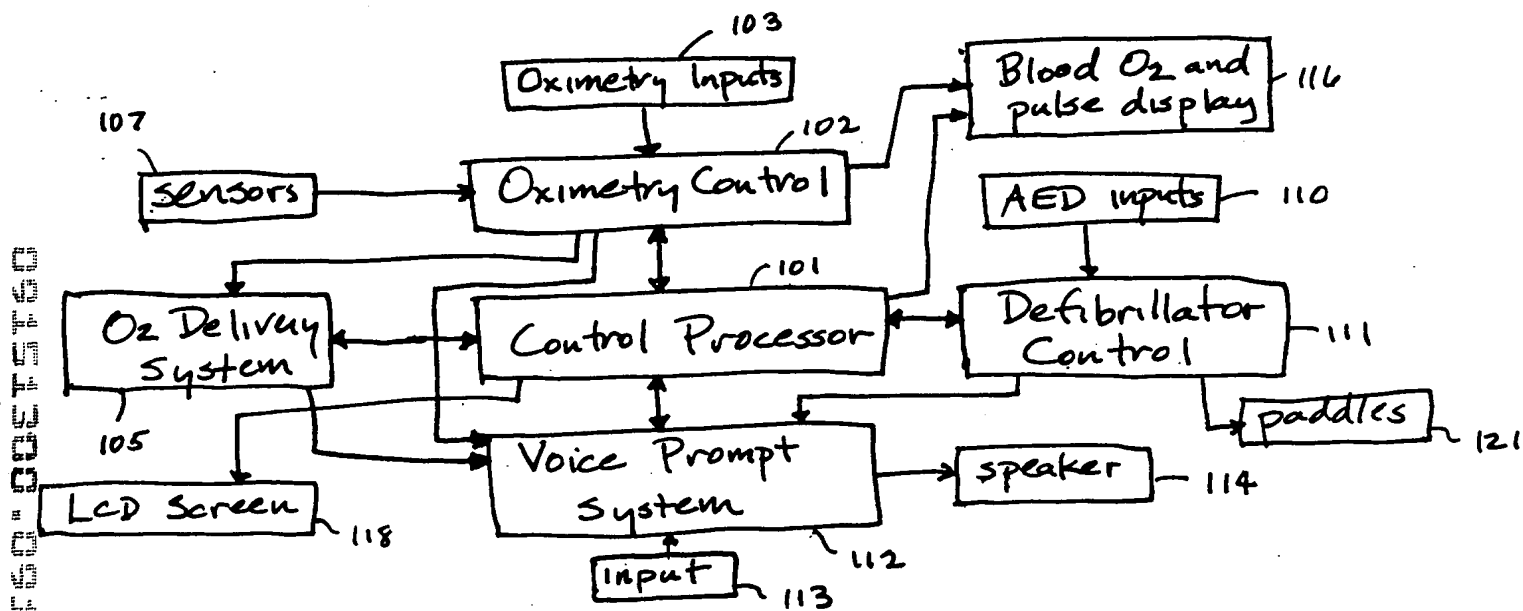


Fig. 4